

Account Information

---

Date Account Number

---

Account Name Contact Name

---

Phone Fax

---

Email Address

---

PO Number Mark For

---


Name

---

Address

---

City State Zip

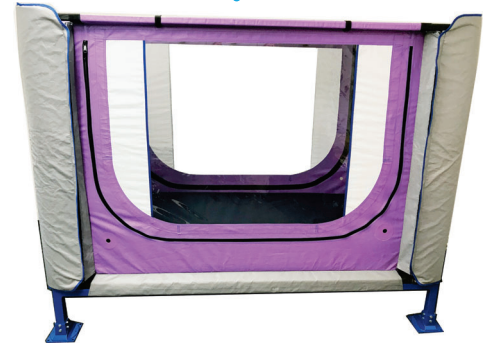

Each Safespace is custom fabricated. The image above is an example of multiple custom selections.

**Safespace Sleeping Compartment**

For individuals who require the safety of a full enclosure, but no hi-lo function, the Safespace Sleeping Compartment offers the robust safety enclosure of the Safespace, with an elevated surface for easy transfers. Hard surfaces are not padded like other products, the design prevents any contact with hard surfaces whatsoever. E1399\*\*





























**AI 109** \$29,801 Safespace Sleeping Compartment with standard mattress with PVC cover, main zip opening w/ viewing panel. Solid back wall. Viewing panel in head and foot end, water resistant floor seams. Configuration selections required below.

**SELECT** Mattress to Floor Height:  18"  24"

<b>ONE selection per side/end is REQUIRED:</b>	<b>Main Side</b>	<b>Opposite Side</b>	<b>Head End</b>	<b>Foot End</b>
Roll up wall w/ Viewing Panel ( <b>Option 1</b> See pg 3)	<input type="checkbox"/> N/C	AI 28 <input type="checkbox"/> \$1,131	N/A	N/A
Nursing Flap ( <b>Option 2</b> See pg 3)	AI 32 <input type="checkbox"/> \$754	AI 28 \$1,131 + AI 32 \$754	N/A	N/A
Frequent Access Opening ( <b>Option 3</b> See pg 3)	AI 96 <input type="checkbox"/> \$565	AI 28 \$1,131 + AI 96 \$565	N/A	N/A
Nursing Flap & Frequent Access Opening ( <b>Option 4</b> See pg 3)	AI 32 \$754 + AI 96 \$706	AI 28 \$1,131 + AI 32 \$754 + AI 96 \$706	N/A	N/A
Solid wall without Viewing Panel ( <b>Option 5</b> See pg 3)	N/A	<input type="checkbox"/> N/C	<input type="checkbox"/> N/C	<input type="checkbox"/> N/C
Non-Opening Viewing Panel ( <b>Option 6</b> See pg 3)	N/A	AI 29 <input type="checkbox"/> \$706	<input type="checkbox"/> N/C	<input type="checkbox"/> N/C
'D' shaped Zip Opening w/ Viewing Panel ( <b>Option 7</b> See pg 3)	N/A	N/A	AI 31 <input type="checkbox"/> \$565	AI 31 <input type="checkbox"/> \$565

Memory Foam Mattress Upgrade	AI 108	<input type="checkbox"/>	\$539	** Not suitable for individuals with chewing or biting behaviors.
Foam Wedge and Cylinder 30° (20" tall x36" wide) (9" dia. x 36" wide)	AI 68	<input type="checkbox"/>	\$2,683	
Foam Wedge Only 30° (20" tall x 36" wide)	AI 69	<input type="checkbox"/>	\$1,718	
Foam Cylinder Only (9" dia. x 36" wide)	AI 70	<input type="checkbox"/>	\$964	
Water Resistant Wall Seams	AI 101	<input type="checkbox"/>	\$905	


**COLORS** (All colors are approximate, variations to be expected)

Wall Color (Req)	Floor Color (Req)	PVC Mattress Color (Req)	Lycra Mattress Color (Optional)	External Corner Color (Req)
 Light Blue <input type="checkbox"/>	 Dark Blue <input type="checkbox"/>	 Dark Blue <input type="checkbox"/>	 Black <input type="checkbox"/>	 Light Blue <input type="checkbox"/>
 Light Pink <input type="checkbox"/>	 Fuchsia <input type="checkbox"/>	 Fuchsia <input type="checkbox"/>	*This is the top 1/2 color. Bottom 1/2 is PVC Mattress Color selected left. NOT SUITABLE FOR USERS WHO HAVE BITING/CHEWING BEHAVIORS.	 Light Pink <input type="checkbox"/>
 Gray <input type="checkbox"/>	 Plum <input type="checkbox"/>	 Plum <input type="checkbox"/>		 Gray <input type="checkbox"/>
 Lilac <input type="checkbox"/>	 Dark Green <input type="checkbox"/>	 Dark Green <input type="checkbox"/>	*If selecting Lycra Mattress Upgrade, this is the bottom 1/2 color.	 Lilac <input type="checkbox"/>
 Light Green <input type="checkbox"/>				 Light Green <input type="checkbox"/>
 Sand <input type="checkbox"/>				 Sand <input type="checkbox"/>
 Cream <input type="checkbox"/>				 Cream <input type="checkbox"/>
 Aqua <input type="checkbox"/>				 Aqua <input type="checkbox"/>
				 Dark Blue <input type="checkbox"/>
				 Fuchsia <input type="checkbox"/>
			 Plum <input type="checkbox"/>	

## Main Side and Opposite Side Configurations


### Option 1

The zip is slightly below the top of the mattress. This is the **standard** opening for the **main** side and **optional** for the **opposite side**. (AI 28)

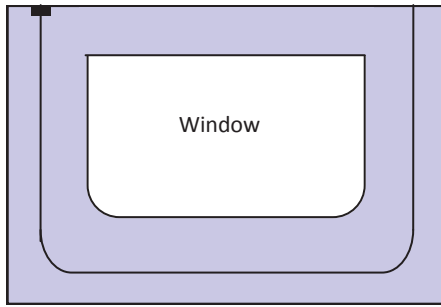


### Option 2

The main zip is slightly below the top of the mattress. The nursing access panel zip is 6" above the top of the mattress. (AI 32)

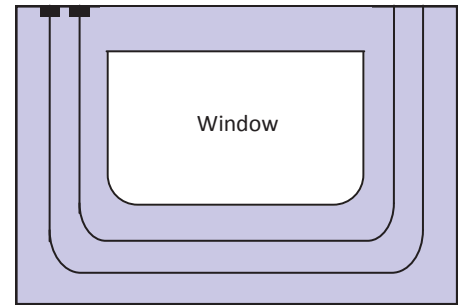


### Option 3

The main zip is slightly below the top of the mattress. The frequent access opening zip is 8" above the top of the mattress and opens 20" along the mattress length. (AI 96)

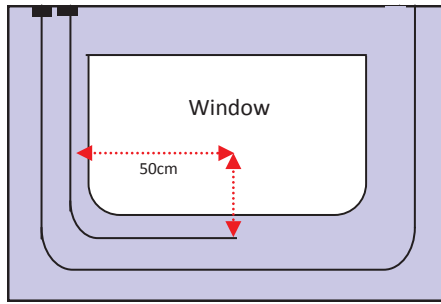

### Option 4

The main zip is slightly below the top of the mattress. The nursing access panel zip is 6" above the top of the mattress. The frequent access opening zip is 8" above the top of the mattress and opens 20" along the mattress length. (AI 32 + AI 96)

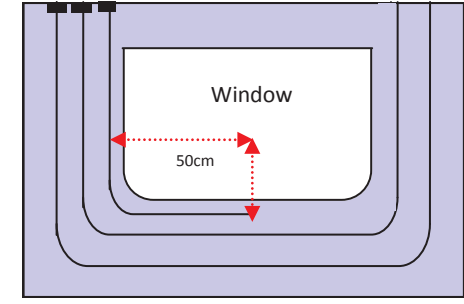


### Option 5

The standard configuration of the opposite side is a solid wall without window.



### Option 6


Non Opening viewing panel along opposite side. (AI 29)

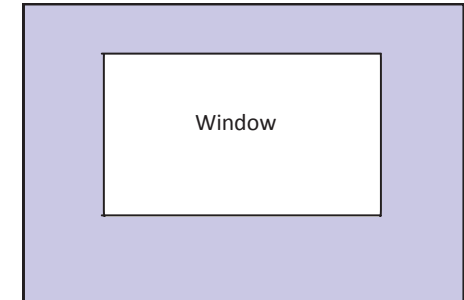

## Head and Foot End Configurations


### Option 5

Optional solid wall in head or foot end for a lower stimulation environment. (No Charge)




### Option 6

Standard configuration of Head and Foot end. Non opening viewing panel.




### Option 7

Optional 'D' shaped zip opening for Head and/or Foot end. (AI 31)



**Tube Hole Options**

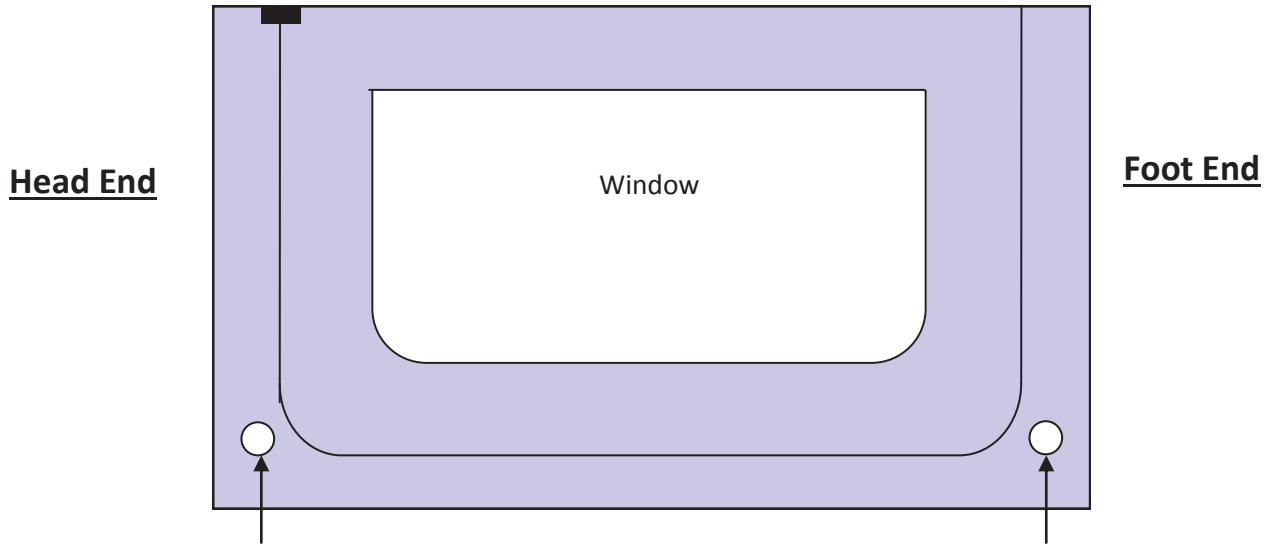

**Example of tube hole positioning on the main panel.**

**Options for tube holes:** Tube holes will be made 1" diameter unless you otherwise specified.

AI 30 Tubing Holes 1" each    1  2  3  4  5  6     \$118 ea

Which panel on are the tube holes to be positioned?	Number of tube holes required	Diameter if different to standard 1"
Front Panel- head end		
Front Panel- foot end		
Back Panel- head end		
Back Panel- foot end		

AI 20 Zip Covers    1  2  3  4  5  6     \$118 ea

Zip covers can be sewn on one end of the zipper seam inside the compartment to prevent the occupant from accessing the backside of the zipper. Describe locations below.

## Specifications

### Internal dimensions \*

- Internal dimensions: 78" x 36"
- Internal height foam floor to ceiling = 50"
- Internal height top of mattress to ceiling= 44"
- Mattress thickness: 6"
- \*Custom Sizes available

### External dimensions

- 18" mattress height: 84"L x 46"W x 65"H
- 24" mattress height: 84" L x 46"W x 71"H

### Roll up Wall Opening

- Length: 62"
- Height: 41"

### Base Clearance

- 18" mattress height has 10" clear space under frame.
- 24" mattress height has 16" clear space under frame.

### Clearance required from hard surfaces

- From top of external frame to room ceiling: 6"
- The front and rear opening panels need to be positioned at least 22" away from any wall or other hard surfaces
- The head and front panels need to be positioned at least 10" away from any wall or other hard surfaces
- Minimum room ceiling height required: 93"

### Safe Working Load

- 396 lbs

\*\*It is the responsibility of the CRT provider to determine the HCPCS code most appropriate for each circumstance. The HCPCS codes for reference only and are not to be deemed as legal advice. Actual coding and coverage varies by funding entities and the use of HCPCS does not guarantee coverage or payment.